

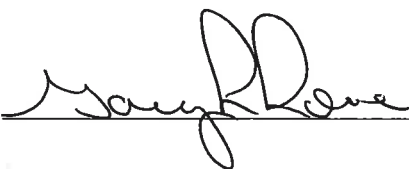
FEB 0 4 2011  
2011  
3/9/11

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

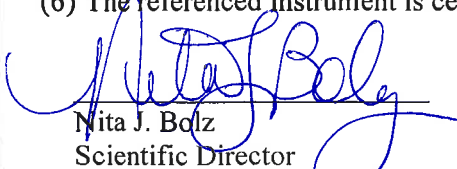
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130174	ow 2/4/11
A	Name	Lowe, Gary	ID#	7219 ✓
	Date	1/31/2011 ✓	Phone #	766-2121
	Agency	Haines Police		
	Instrument Location	Haines Police		
B	Alco S/N	X301526 ✓	Target Value	.078 ✓
			High Pressure	500
	Alco Test Values	.081 ✓		.080 ✓
		1 <sup>st</sup> Alco		2 <sup>nd</sup> Alco
	Signature			
		(OVER)		


8mb  
2/8/11


I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 14<sup>th</sup> day of MAR 2011

  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130174

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130174

JANUARY 31, 2011

OPERATOR'S NAME:

LOWE, GARY

OPERATOR'S NUMBER: 7219

SUBJECT'S LAST NAME:

VERIFY

SUBJECT'S FIRST NAME/NI:

VERY

O.L. #: 01312011

DEPT/AGENCY: HNS1

CASE/REPORT: 01-31-2011

TEST TYPE: V

ALCO TARGET VALUE: .078

ALCO S/N: K301526

— BREATH ANALYSIS —

.078 ADJUSTED FOR 30.58 in

ALCO TARGET	.079	13:45
BLANK TEST	.000	13:46
INTERNAL STANDARD	VERIFIED	13:46
ALCO TV 30.58 in	.081	13:46
BLANK TEST	.000	13:47
SUBJECT SAMPLE	.000	13:47
BLANK TEST	.000	13:48
ALCO TV 30.58 in	.000	13:48
BLANK TEST	.000	13:49

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130174

JANUARY 31, 2011

TIME 13:50

— DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	30.58 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#&'()\*+,-./0123456789:;<=>?@ABCDEF  
GHIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefg  
hijklmnopqrstuvwxyz{|}~